






Intrada Organic Acid

150 x 2 mm

HPLC COLUMN APPLICATION

LC-MS: Nucleoside triphosphate (NTP)

ヌクレオシド三リン酸の LC-MS 分析

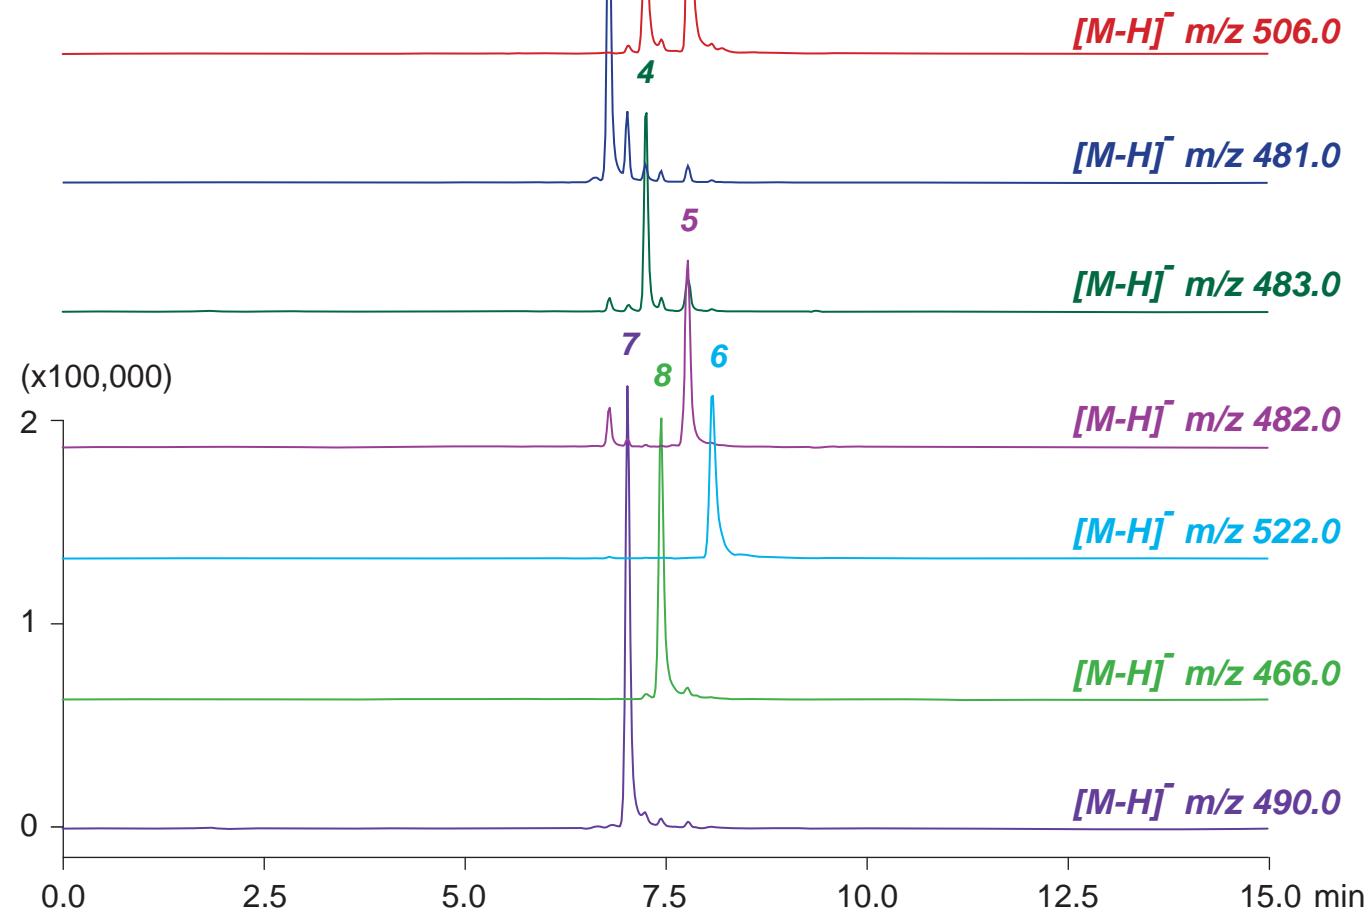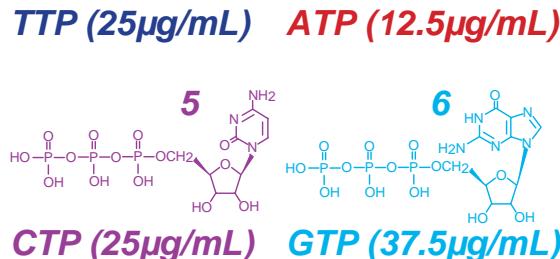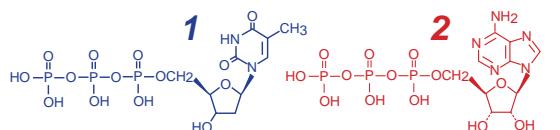

Intrada Organic Acid, 150 x 2 mm

A: acetonitrile / 100mM ammonium acetate = 95 / 5

B: acetonitrile / 100mM ammonium acetate = 10 / 90

15-75% B (0-9min), 100% B (9-15min)

0.2mL/min (6MPa), 60°C, 5 μ L (12.5-37.5 μ g/mL, 1%HCOOH)

MS (ESI, SIM, Negative)