

Nardis ND-NX


Unison UK-Amino

150 x 4.6 mm

HPLC COLUMN APPLICATION

Urea, allantoin

尿素、アラントイン

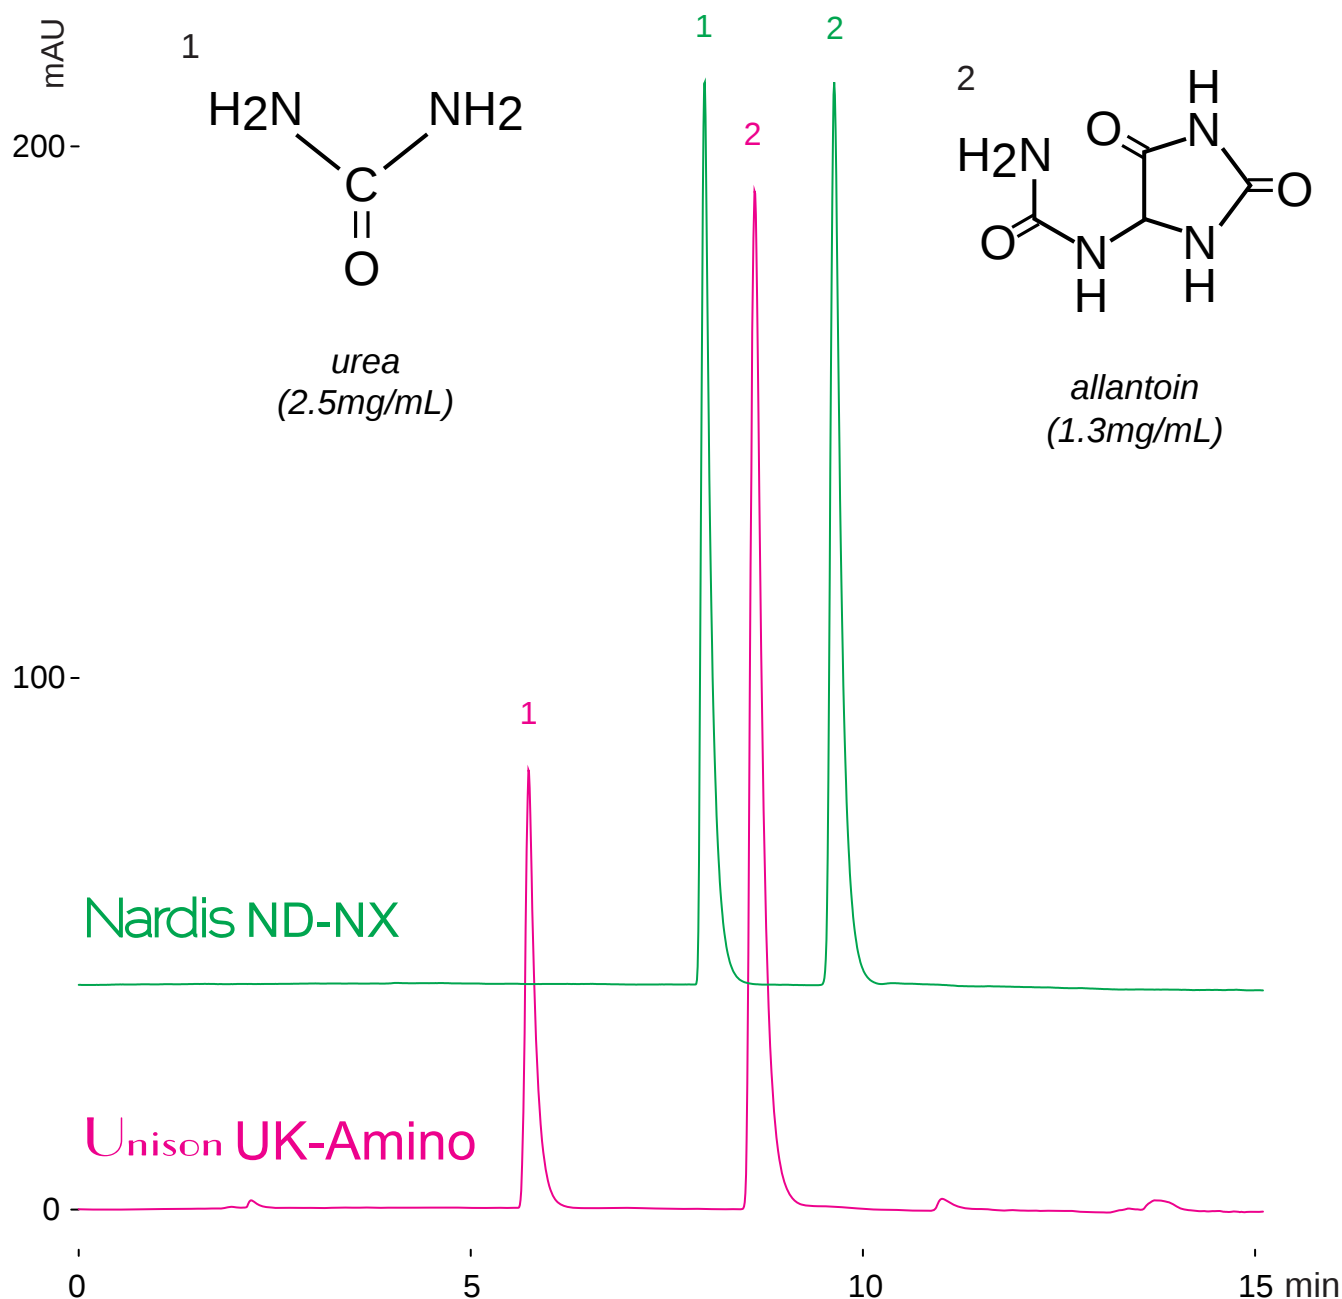

150 x 4.6 mm

A: acetonitrile

B: 100mM ammonium acetate

0-40%B (0-15min)

1.0mL/min (6MPa), 37°C

ELSD (spray chamber 70°C, drift chamber 70°C)

10μL (1.3-2.5mg/mL, water/methanol=50/50)