

**Intrada Amino Acid**

150 x 3 mm



Application

**LC-TOFMS: Urinary compounds**



尿代謝関連化合物のLC-TOFMS分析

Metabolomics Core Facility, McGill University  
GB 2017/06/16

**Argininosuccinic acid [M+H]<sup>+</sup>: 291.1299**

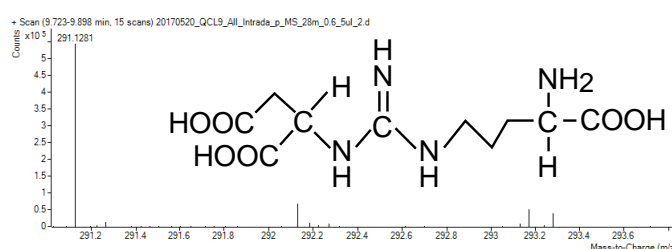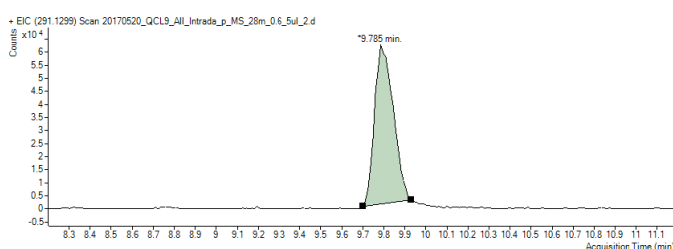

**Methylnicotinamide [M+H]<sup>+</sup>: 137.0709**

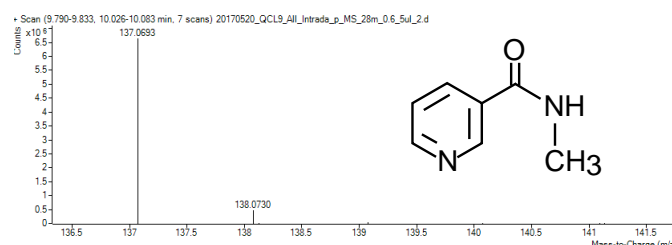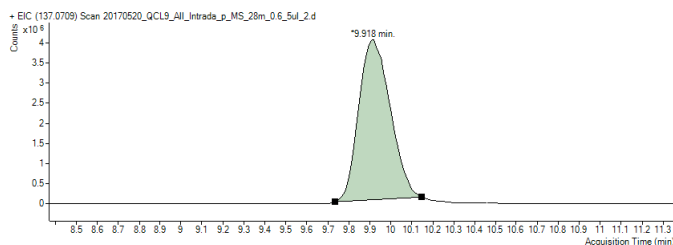

*Intrada Amino Acid, 150x3mm*

A) ACN /HCOOH = 100 / 0.3, B) 100mM HCOONH<sub>4</sub> in 20% ACN / 80% water  
0-27%B (0-3min), 27-100%B (3-19.5min), 100%B (19.5-25min), 0%B (25-32min)  
0.6 mL/min, 10°C, 5µL (ca. 1mM in water)

Agilent 1290 Infinity UHPLC - 6540 UHD Accurate-Mass Q-TOF mass spectrometer (ESI<sup>+</sup>)

Courtesy of Dr.Gaelle Bridon and Dr.Daina Avizonis, McGill University, CANADA