

Nardis ND-NX


Unison UK-Amino

250 x 4.6 mm

HPLC COLUMN APPLICATION

Sugar alcohols

糖アルコール類の分析

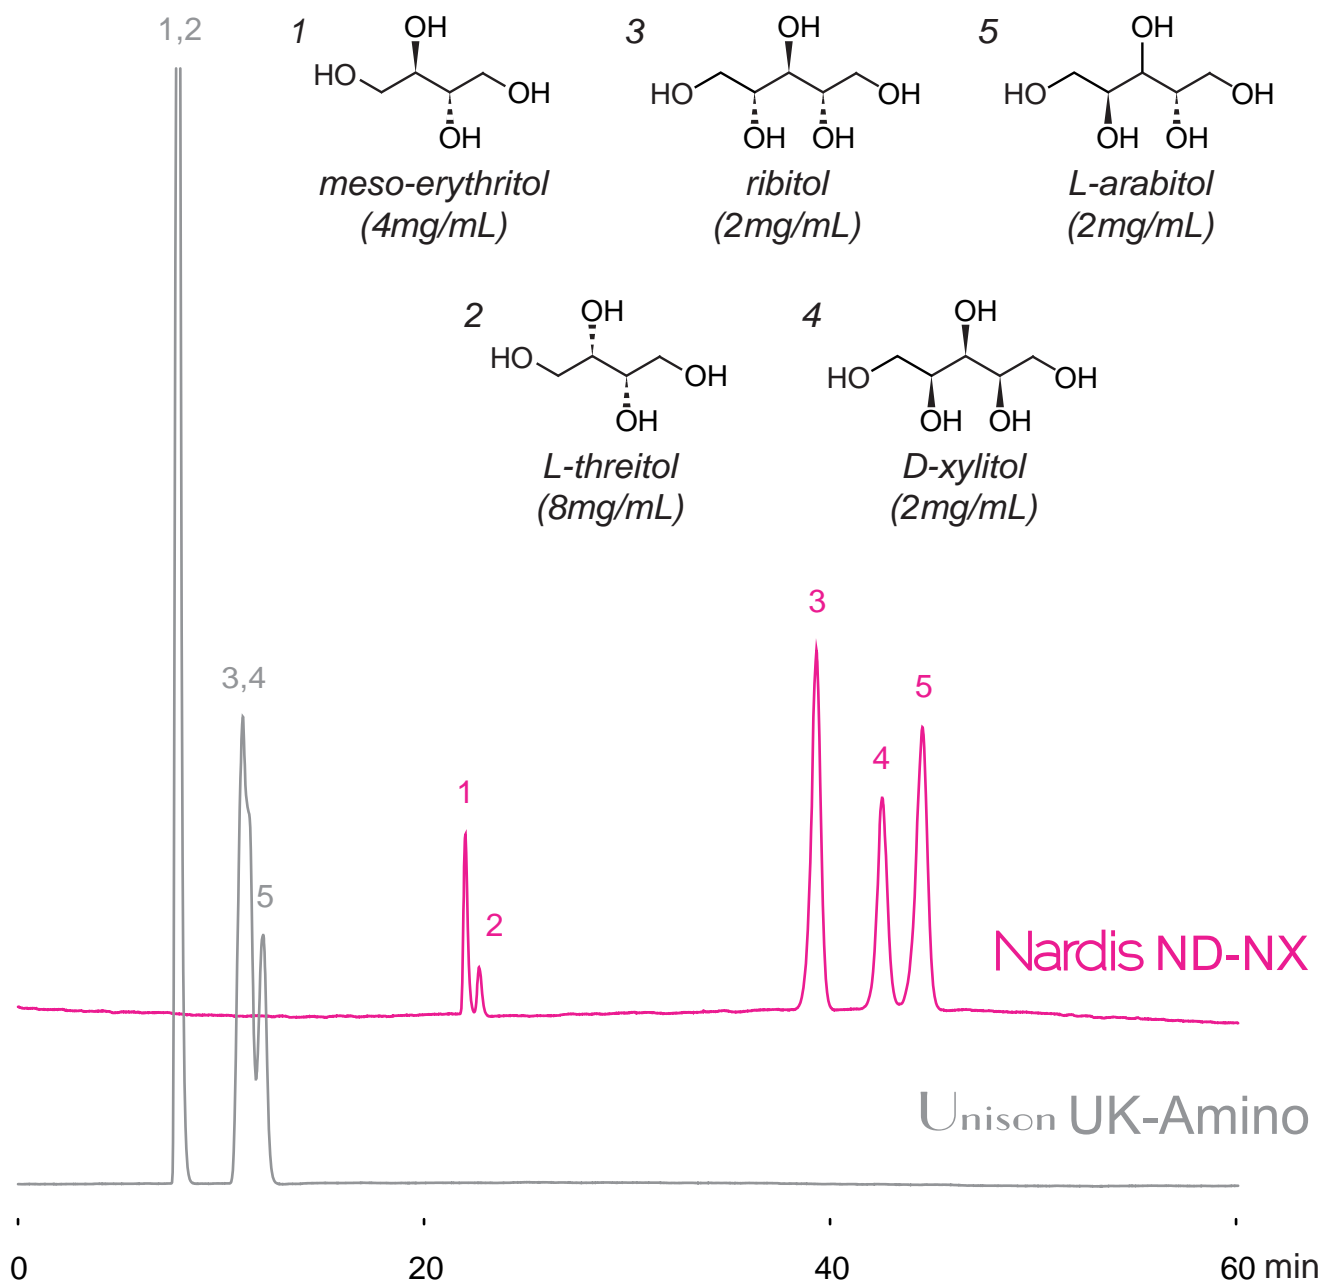

250 x 4.6 mm

A: acetonitrile

B: 10mM ammonium acetate

5-10%B (0-60 min), 1.0 mL/min, 60°C

ELSD (spray chamber 70°C, drift chamber 100°C)

10 µL (2-8mg/mL, water)