


Scherzo SS-C18

250 x 4.6 mm

HPLC COLUMN APPLICATION

Pyrimidine isomers

ピリミジン異性体

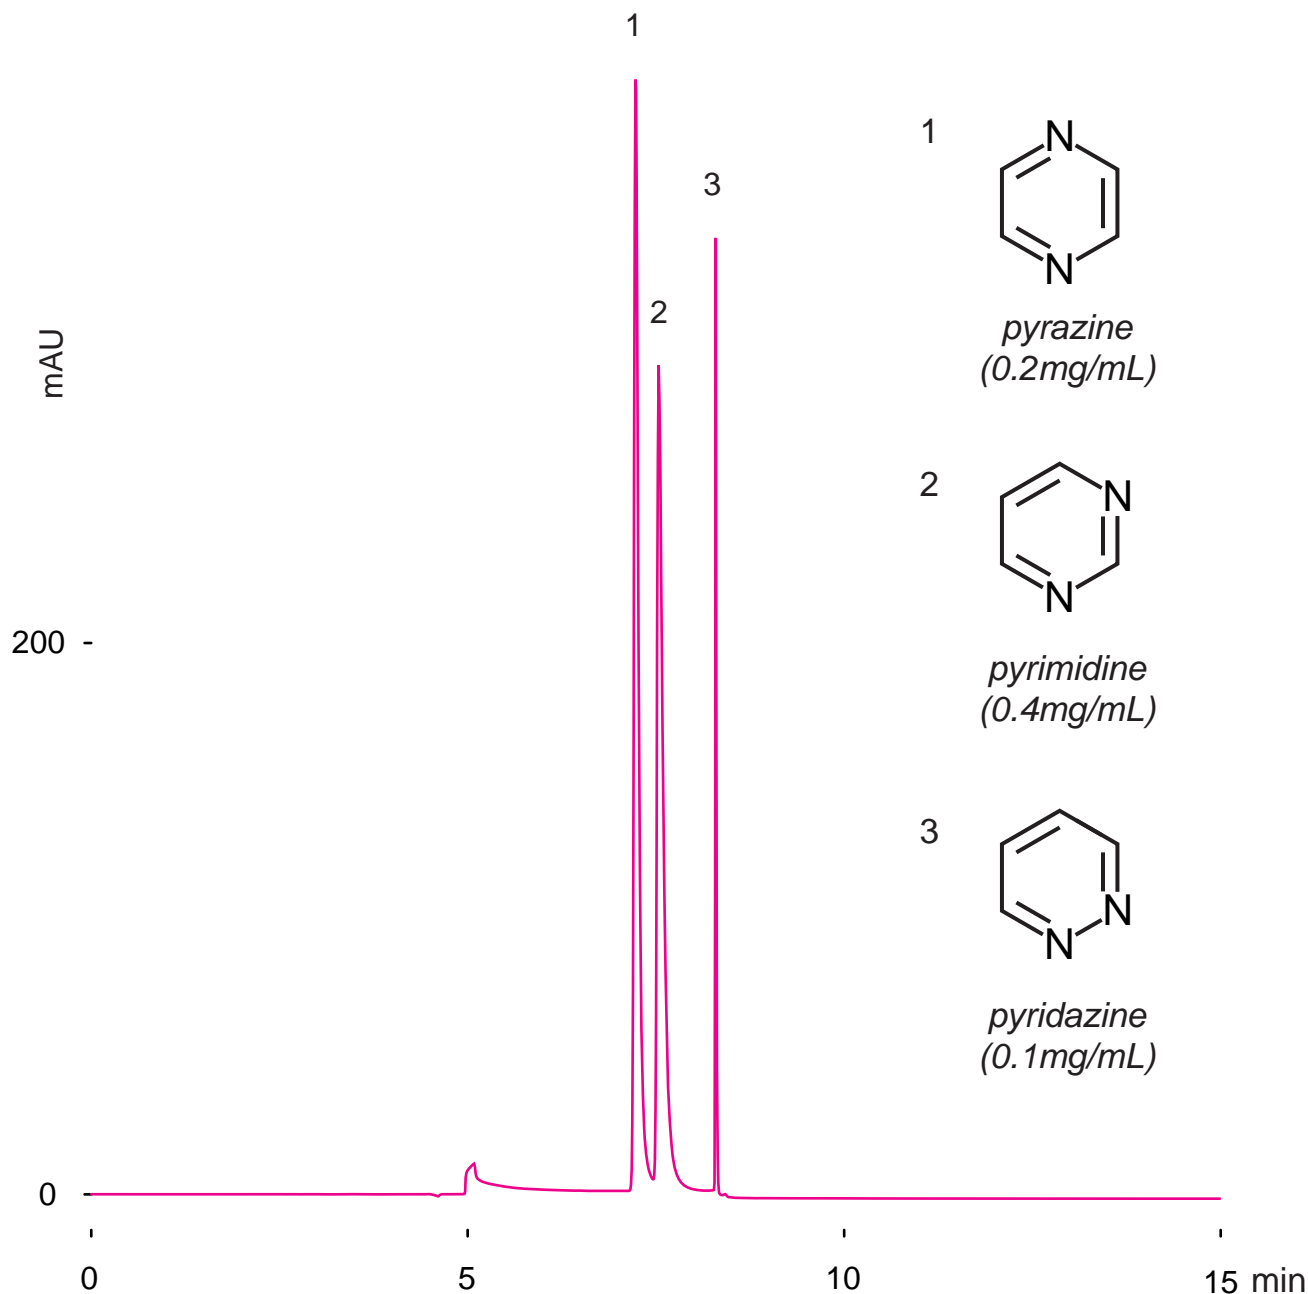

Scherzo SS-C18, 250 x 4.6 mm

A: water / acetic acid = 100 / 0.5

B: 50mM ammonium acetate / acetonitrile = 80 / 20

0-50%B (0-4min), 50%B(4-25min)

1.0mL/min (16MPa), 37°C, 250nm

10µL (0.1-0.4mg/mL, water)