


Nardis ND-NX

Unison UK-Amino

250 x 4.6 mm

HPLC COLUMN APPLICATION

DL-glyceraldehyde, dimer
DL-グリセルアルデヒド、二量体の分析

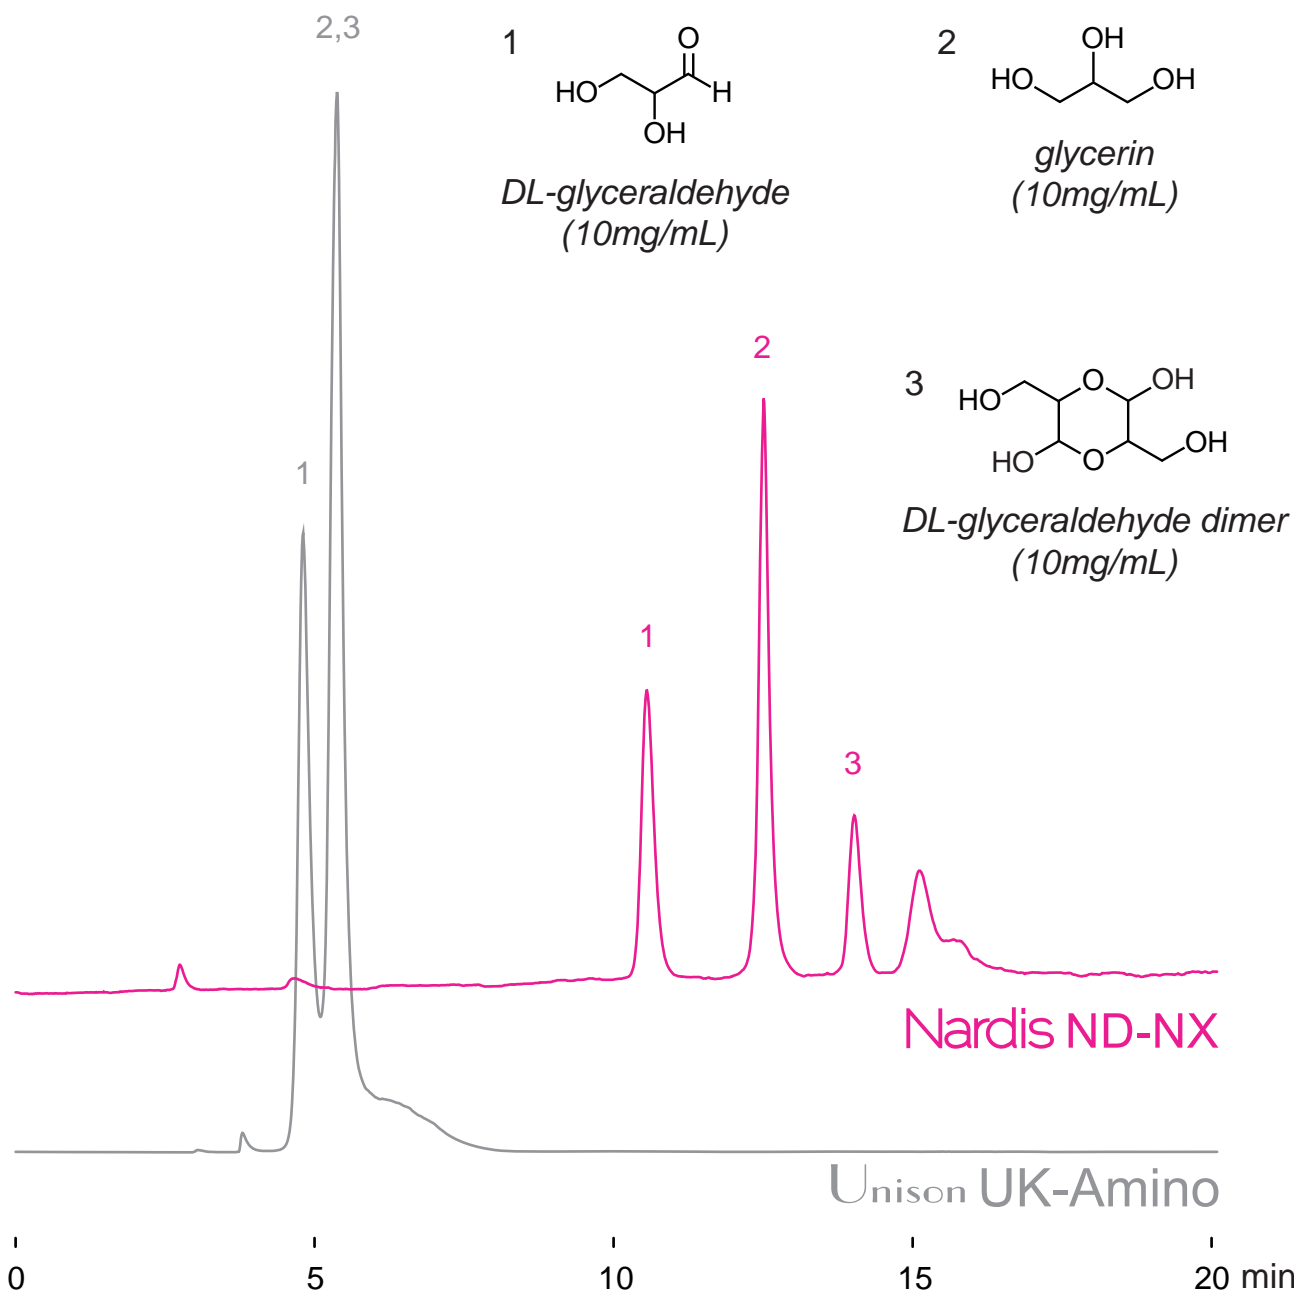

250 x 4.6 mm

A: acetonitrile

B: acetonitrile / 100mM ammonium acetate = 50 / 50

15-25%B (0-20 min), 100%B (20-25 min)

1.0 mL/min (7MPa), 60°C

ELSD (spray chamber 60°C, drift chamber 60°C)

10 µL (1.0mg/mL, water/HCOOH=100/1)