

Cadenza CW-C18


Presto FF-C18

250 x 4.6 mm

HPLC COLUMN APPLICATION

Phycocyanin from Spirulina

フィコシアニン (スピルリナ由来)

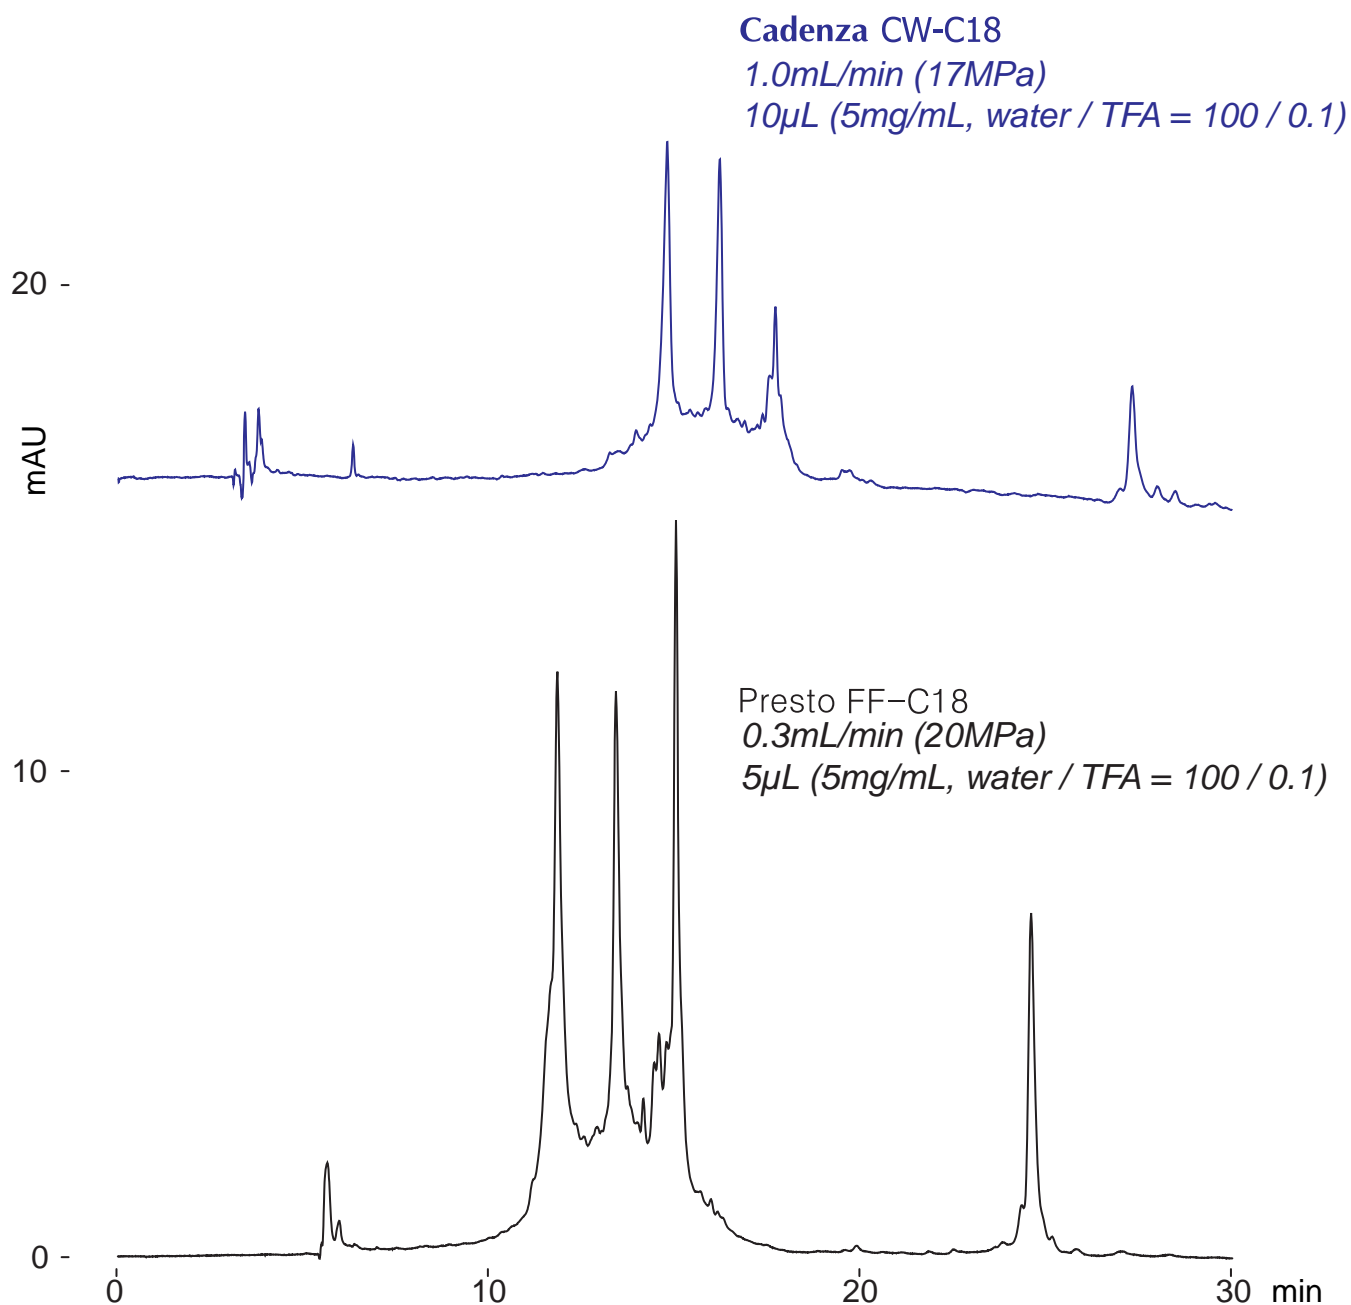

250 x 4.6 mm

A: water / trifluoroacetic acid = 100 / 0.1

B: acetonitrile / trifluoroacetic acid = 100 / 0.07

45-70%B (0-30min)

37°C, 620nm